


Calibrate Thermometers Often!

Make sure temperatures are accurate

Ice water method

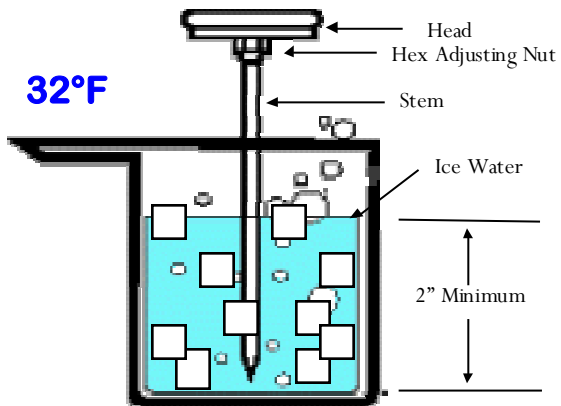

Wait 30 seconds




Adjust



Hold 30 seconds
Recheck

Boiling water method

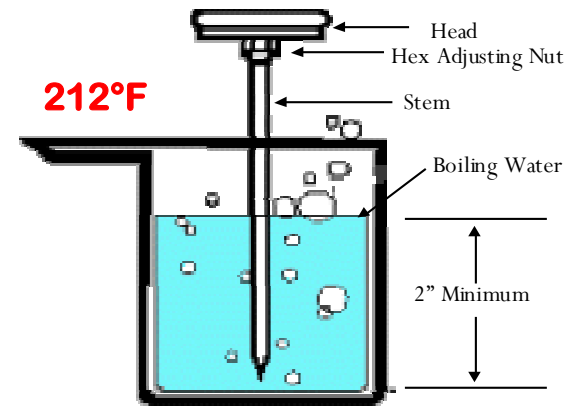

Wait 30 seconds

What to do

- ⊕ Fill a large glass with crushed ice.
- ⊕ Add clean tap water until glass is full.
- ⊕ Put the thermometer or probe stem into the ice water so that the sensing area is completely submerged.
- ⊕ Wait 30 seconds. **32°F**
- ⊕ Hold the adjusting nut securely with a wrench or pliers and rotate the head of the thermometer until it reads 32°F.

Notes

- ⊕ Stir the mixture well
- ⊕ Do not let the stem touch the bottom or sides of the glass.
- ⊕ The thermometer stem or probe stem must remain in the ice water.
- ⊕ Press the reset button on a digital thermometer to adjust the readout.

What to do

- ⊕ Bring clean tap water to a boil in a deep pan.
- ⊕ Put the thermometer or probe stem into the boiling water so that the sensing area is completely submerged.
- ⊕ Wait 30 seconds. **212°F**
- ⊕ Hold the adjusting nut securely with a wrench or pliers and rotate the head of the thermometer until it reads 212°F (100°C) or the appropriate boiling temperature.

Notes

- ⊕ Do not let the stem touch the bottom or sides of the pan.
- ⊕ The thermometer stem or probe stem must remain in the boiling water.
- ⊕ Press the reset button on a digital thermometer to adjust the readout.



FOOD SAFETY PROGRAM(216)
201-2000

CUYAHOGA COUNTY
BOARD OF HEALTH